

**BUREAU OF INDIAN STANDARDS**  
**DRAFT FOR COMMENTS ONLY**

Doc No.: PGD 21 (24862) WC  
IS 5235 : 2024

---

*भारतीय मानक मसौदा*

**मौसम विज्ञान — वर्षामापी, अभिलेखन — विशिष्टि**  
(IS 5235 का दूसरा पुनरीक्षण)

*Draft Indian Standard*

**Meteorology — Raingauges, Recording — Specification**  
(*Second Revision of IS 5235*)

ICS 07:060

Not to be reproduced without permission of BIS or use as Standard	Last date for receipt of comment is 30-06-2024
--	---

Meteorological Instruments Sectional Committee, PGD 21

## FOREWORD

*(Formal Clauses will be added later)*

The recording raingauge consists of a collector and a rainfall recording mechanism mounted on a base. The rainfall measuring unit consists of a float chamber containing a light metal float and a siphon chamber. Rain from the collector is led into the float chamber through an inlet tube and as the float rises, a pen fixed to the float rod draws a line on a chart wound on a rotating drum driven by clockwork. The discharge tube is inside and coaxial with the outer tube of the siphon chamber. The top of this outer tube has a polished glass cap and the discharge tube comes to within a very short distance of this. When the level of water in the outer tube rises with that of the water in float chamber and flows over the bend, capillary action causes all the air to be pushed out and down the delivery tube so that a full, flow is started at once. Similarly, at the end of the siphoning, once air gets to the top of the tube the siphoning action is stopped immediately. When siphoning occurs, the pen fixed on the float rod falls to the zero mark on the chart and the gauge is ready to record rainfall again.

This standard was originally published in 1969 and subsequently revised in 1992. This revision has been taken up to keep pace with the latest technological developments and international practices. In this revision following major changes have been made:

- a) UDC number has been replaced by ICS number on first cover page;
- b) Reference clause has been updated;
- c) The grade of aluminium alloy for the rim of the collector has been updated in accordance with the latest edition of IS 617;

- d) In **4.1(b)**, the word ‘animal’ has been deleted; and
- e) Fig. 1 has been modified based on an improved model of recording raingauge.

For the purpose of deciding whether a particular requirement of this standard is complied with, the final value, observed or calculated, expressing the result of a test or analysis, shall be rounded off in accordance with IS 2: 2022 ‘Rules for rounding off numerical values (*second revision*)’. The number of significant places retained in the rounded off value should be the same as that of the specified value in this standard.

*Draft Indian Standard*  
**METEOROLOGY — RAINGAUGES, RECORDING — SPECIFICATION**  
*(Second Revision)*

## 1 SCOPE

This standard specifies the requirements for natural siphon type recording raingauges.

## 2 REFERENCES

The standards listed below contain provisions which, through reference in this text, constitute the provisions of this standard. At the time of publication, the editions indicated were valid. All standards are subject to revision, and parties to agreements based on this standard are encouraged to investigate the possibility of applying the most recent editions of the standards listed below.

<i>IS No.</i>	<i>Title</i>
IS 617 : 1994	Cast aluminum and its alloys - Ingots and castings for general engineering purposes – Specification ( <i>third revision</i> )
IS 2932 (Part 1) : 2013	Enamel, synthetic, exterior: (a) Undercoating (b) Finishing - Specification (Fourth Revision)
IS 4849 : 1992	Meteorology — Rain measures — Specification ( <i>first revision</i> )
IS 5924 : 1988	Clock mechanisms and drums for meteorological instruments ( <i>first revision</i> )
IS 5947 : 1970	Charts for recording meteorological instruments

## 3 TYPES

The recording raingauges shall be of following types depending on the intensity of the rainfall to be measured:

- a) Recording raingauge for 10 mm rainfall, natural siphon recording raingauge having a collector 325 cm<sup>2</sup> in area with a range 0 to 10 mm of rainfall per siphoning, for use in regions of light or medium rainfall, and
- b) Recording raingauge for 25 mm rainfall, natural siphon recording raingauge having a collector 130 cm<sup>2</sup> in area with a range 0 to 25 mm of rainfall per siphoning, for use in regions of heavy rainfall.

## 4 MATERIALS

**4.1** The material used for the fabrication of the collector and base of the recording raingauges shall have the following properties:

- a) Rigidity and strength with no distortion or other deterioration when exposed to widely varying climatic conditions in the open air, while at the same time being light in weight. Suitable ultraviolet inhibitor may be added to increase its durability;
- b) Freedom from attack by insect or fungoid life;
- c) Smooth and permanent surface finish to facilitate free flow of precipitation;
- d) Low thermal conductivity to minimize evaporation losses or condensation gains; and
- e) A life of not less than 15 years in the open.

**4.2** While any material satisfying the requirements as given in **4.1** may be used, glass reinforced polyester is considered as a suitable material.

**4.3** The material used for the manufacture of the recording mechanism shall be gun metal or similar material so that it is capable of being finished to specified dimensions and is not affected in any manner by permanent contact with ordinary water for prolonged periods.

**4.4** The material for the rim of the collector shall be gun metal or aluminium alloy conforming to Grade 4635 of IS 617.

## 5 DIMENSIONS

**5.1** The main dimensions for recording raingauges shall be as given in Fig. 1 and Table 1.

**Table 1 Main Dimensions of Recording Raingauges**

(Clauses 5.1 and 6.3.10)

All dimensions are in millimeters.

Sl No.	Particulars	Raingauge for 10 mm Rainfall	Raingauge for 25 mm Rainfall
(1)	(2)	(3)	(4)
i)	Nominal thickness (base and collector), <i>Min</i>	3	3
ii)	Overall height	675 ± 3	675 ± 3
iii)	Internal diameter of gun metal rim	203 to 203.4	128.5 to 128.6
iv)	Depth of funnel from upper edge of rim, <i>Min</i>	175	175
v)	Internal diameter of funnel outlet pipe	10	10
vi)	Height to which float has to rise from zero for discharge	60.0	60.0
vii)	Diameter of clock drum	93.3	93.3
viii)	Height of drum above flange	92	92

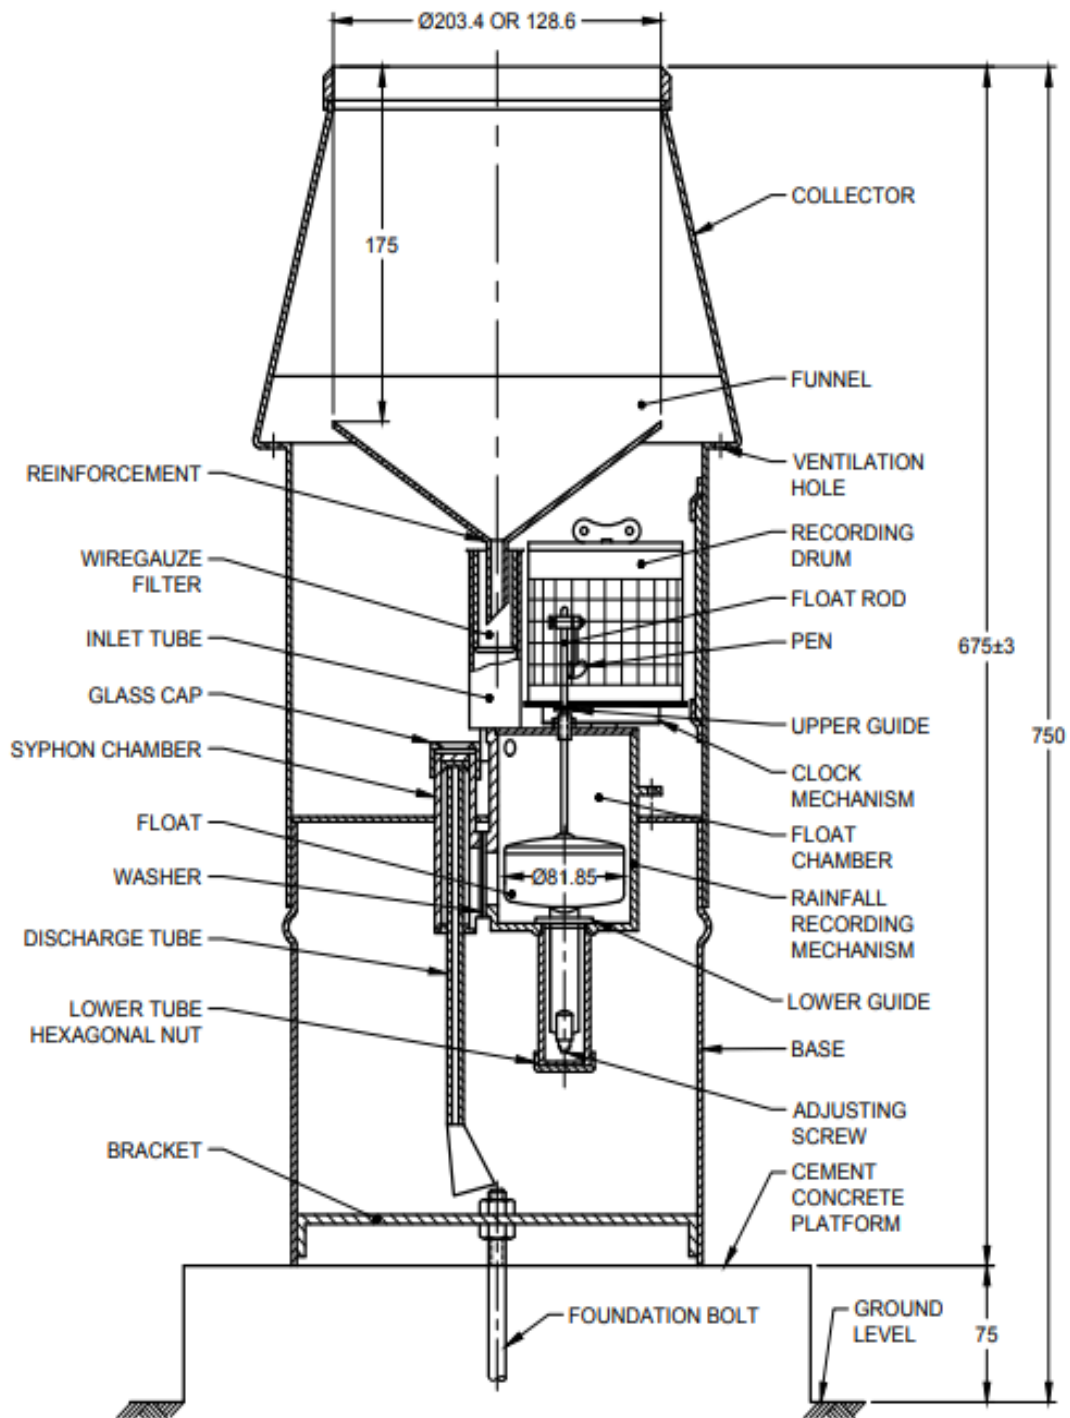


FIG. 1 DIMENSIONS AND NOMENCLATURE OF NATURAL SYPHON RECORDING MECHANISM

**5.2** The inside diameter of the collector rim shall be correct within  $\pm 0.5$  mm of the specified value when measured in any four directions and the mean of the four values shall be within  $\pm 0.2$  mm of the specified value.

## **6 GENERAL REQUIREMENTS**

### **6.1 Collector**

The collector shall have a rim cemented firmly at the top. The rim, having a knife edge, shall be truly circular and have the diameters specified for the two types of raingauges. The inner surface of the rim and the inside vertical wall of the funnel shall be in one plane. The entire inner surface of the funnel shall have a smooth finish. The external shape of the collector shall be slightly tapered with the lesser diameter at top.

**6.1.1** All seams and joints, if any, of the collector shall be of adequate strength and shall be watertight. The junction between the funnel and funnel outlet tube shall specially be reinforced as shown in Fig. 2.

**6.1.2** The collector shall have eight ventilation holes of about 5 mm diameter, drilled at equal distances. The holes shall be covered inside with fine brass mesh and shall be suitably shielded to prevent ingress of water (*see* Fig. 1).

**6.1.3** The collector shall be provided with a cutaway window of  $100 \times 100$  mm so that the chart is visible from outside, without removing the collector. The window shall be covered with a transparent sheet of acrylic plastic which may be slid in grooves framing the window and fixed in position (*see* Fig. 2).

**6.1.4** A suitable rust-proof locking device shall be provided in the collector to lock it to the base.

**6.1.5** The collector shall fit smoothly over the base and rest on it so that when assembled the rim is horizontal.

### **6.2 Base**

**6.2.1** The base shall be strong enough to support without yielding the collector as well as the recording mechanism. The top of the base shall be reinforced for this purpose.


**6.2.2** A strong rust-proof bracket shall be provided at the bottom of the base to enable it to be anchored securely in the cement concrete platform on which the raingauge is permanently fixed.

### **6.3 Recording Mechanism**

The recording mechanism shall be of the natural siphon type, and the design shall be such that the water in the float chamber is emptied immediately and rapidly by the siphon as soon as the specified amount of water has been collected. The complete mechanism shall be water-tight and the siphon action shall start and end sharply. This may conveniently be achieved by interposing in the passage between the float chamber and siphon chamber, a thin disc with a V-shaped opening in it. The disc shall have the dimensions as shown in Fig. 3. The distance between the glass cap at the top of the siphon chamber and the open end of the discharge tube shall  $1.7 \pm 0.1$  mm for a discharge tube having a diameter of 4.7 mm. Two washers, one of suitable packing material and


another of metal above it, shall be provided over the glass disc. They shall have the dimensions given in Fig. 4.

**6.3.1** For both types of raingauges, the discharge of water shall take place soon after the collection of  $324.9 \text{ cm}^3 + 3.2 \text{ cm}^3$  of water corresponding to 10 mm of rainfall in the 10 mm raingauge and 25 mm of rainfall in the 25 mm raingauge. The measuring glasses shall meet the requirements of Type 4 and Type 5 given in IS 4849.

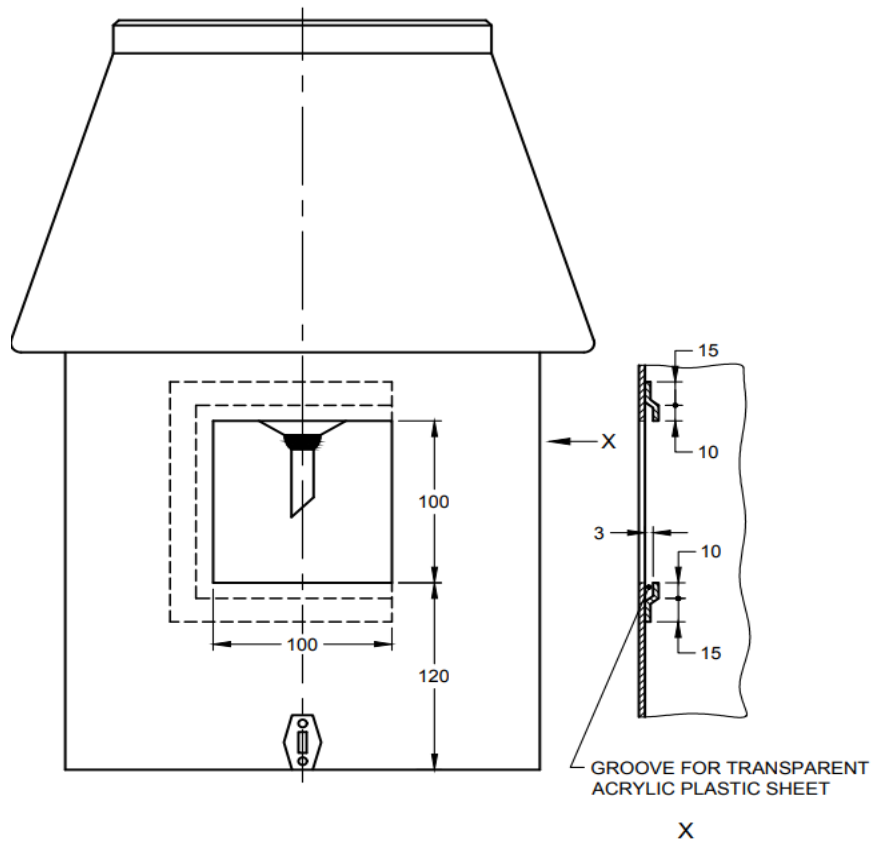


All dimensions are in millimeters.

FIG. 2 WINDOW OF COLLECTOR

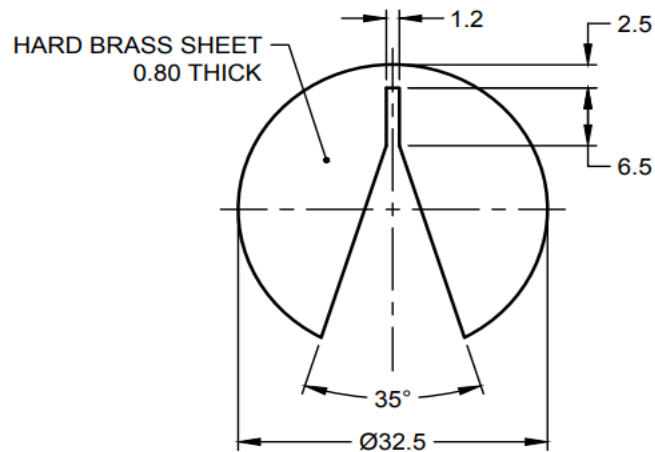

All dimensions are in millimeters.

FIG. 3 DIMENSIONS FOR V-DISC

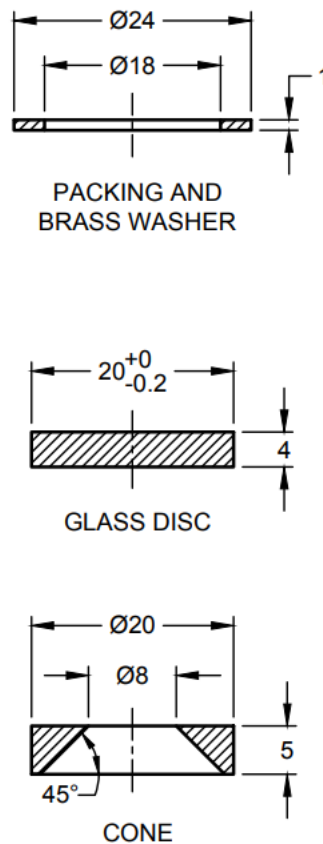

All dimensions are in millimeters.

FIG. 4 DIMENSIONS FOR WASHERS, GLASS DISC AND CONE FOR SYPHON TUBE


**6.3.2** The siphon shall be capable of discharging the collected water and bringing the recording pen back to zero in a period not exceeding 15 s.

**6.3.3** There shall be no dribbling of water before siphoning even when the rate of rainfall is as low as 0.1 mm/h.

**6.3.4** After siphoning, the addition of water equivalent to 0.1 mm of rain in 10 mm raingauge and 0.2 mm of rain in 25 mm raingauge shall produce a perceptible rise of the pen.

**6.3.5** The shape and main dimensions of the float of the recording mechanism shall be as shown in Fig. 5.



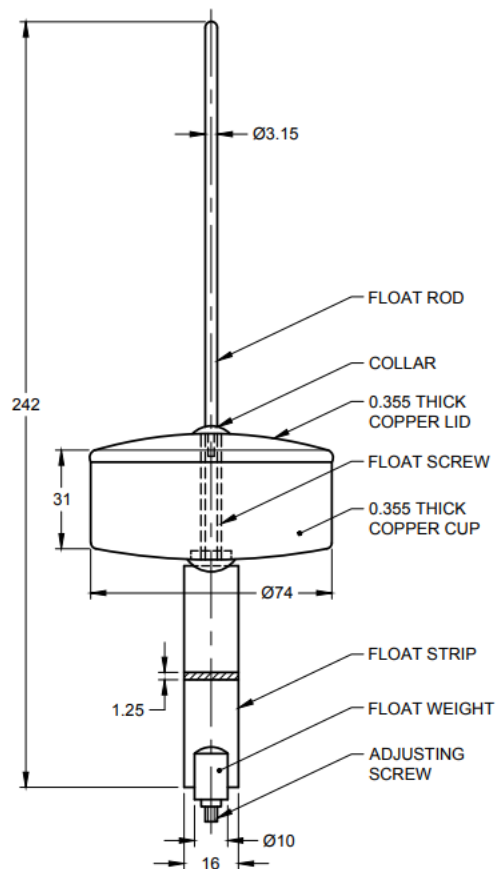


All dimensions are in millimeters.

FIG. 5 DIMENSIONS FOR FLOAT

**6.3.5.1** While other suitable dimensions may also be devised, the following dimensions for the components are found to satisfy the conditions laid down in **6.3.5** (see Fig. 1 and Fig. 5):

- |    |  |              |
|----|--|--------------|
| a) | Internal diameter of the float chamber | 81.85 mm     |
| b) | Total weight of the float chamber      | 94 g to 98 g |

**6.3.5.2** Between the float chamber and the siphon chamber, a suitable packing material washer of the shape and dimensions given in Fig. 6 shall be interposed to prevent leakage of water. The siphon chamber shall be fixed to the float chamber by means of four screws, with provision for adjusting the former for correct siphoning.

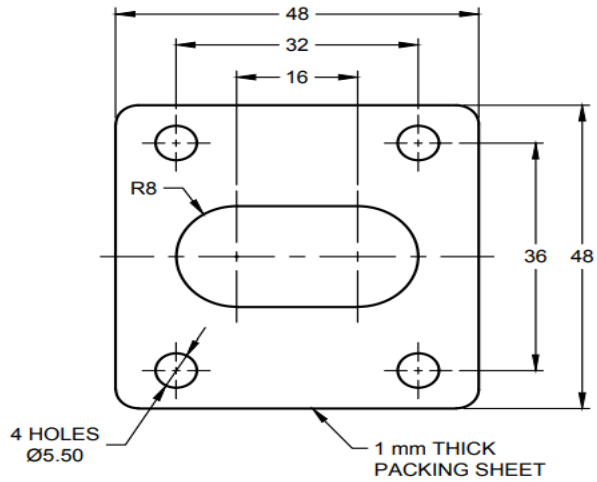


All dimensions are in millimeters.

FIG. 6 PACKING WASHER FOR FLOAT AND SYPHON CHAMBER

**6.3.5.3** The lower end of the float chamber shall be provided with a threaded hexagonal cap, which may be removed for cleaning the float chamber (*see* Fig. 1).


**6.3.6** The wire gauze filter tube shall be a loose fit inside the inlet tube and shall be as shown in Fig. 7.

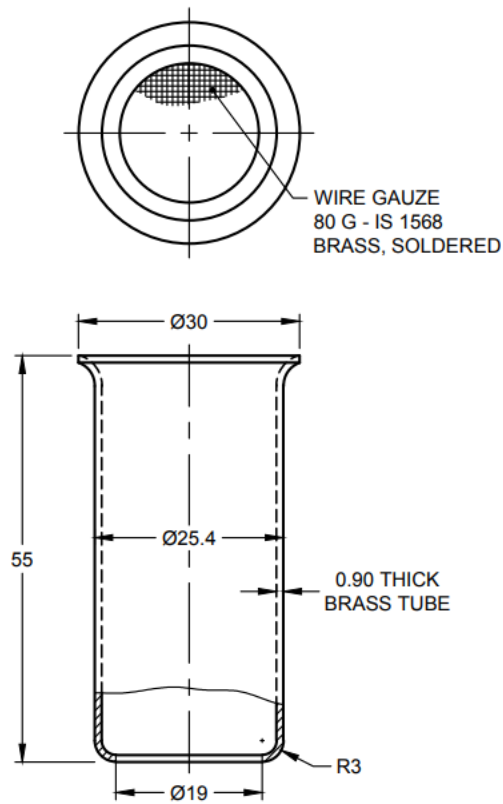



All dimensions are in millimeters.

FIG. 7 WIRE GAUZE FILTER


**6.3.7** The recording pen shall yield a clear trace when moving either vertically or horizontally relative to the chart. It shall be provided with an adjusting screw to permit ready adjustment of zero. It shall have the dimensions as given in Fig. 8(A) or 8(B). A suitable fibre tipped disposable pen can also be used.

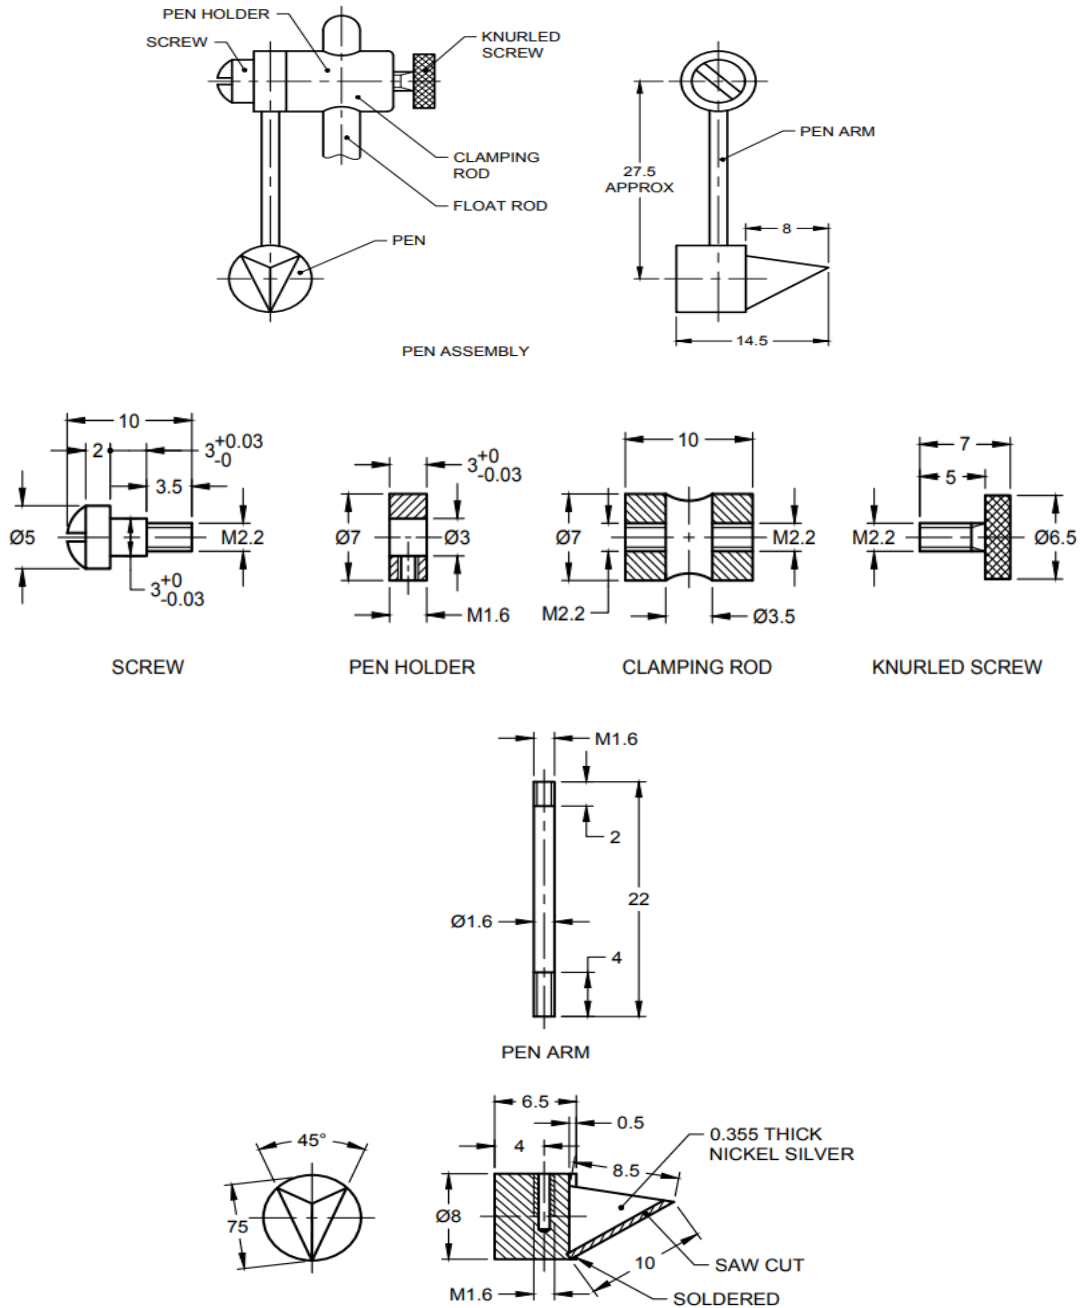


All dimensions are in millimeters.  
**FIG. 8A ASSEMBLY AND DETAILS OF PEN (CONTINUED)**

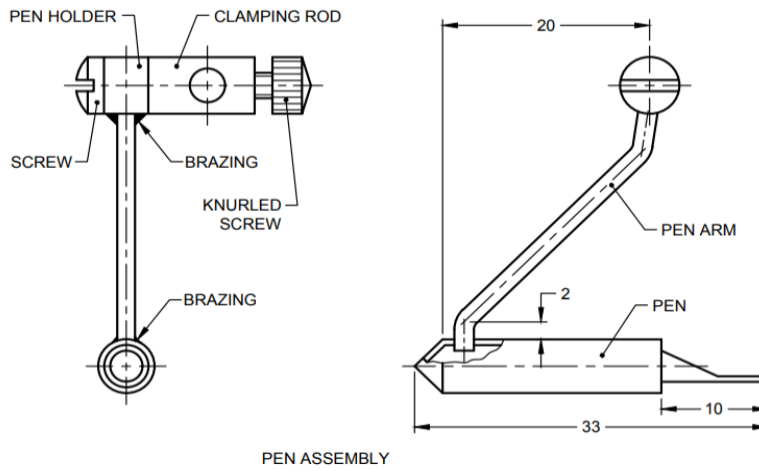


SCREW




PEN HOLDER




CLAMPING ROD



KNURLED SCREW

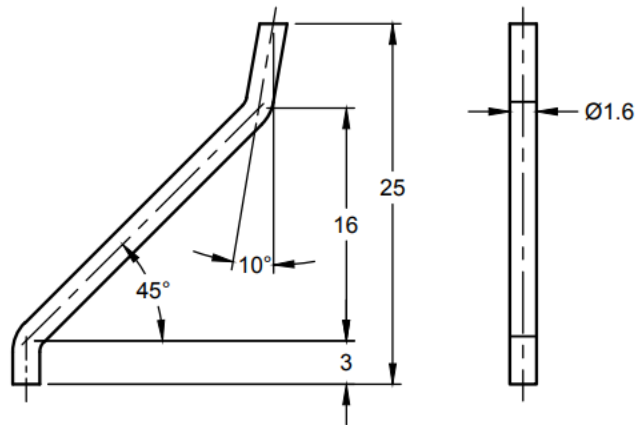

PEN ARM

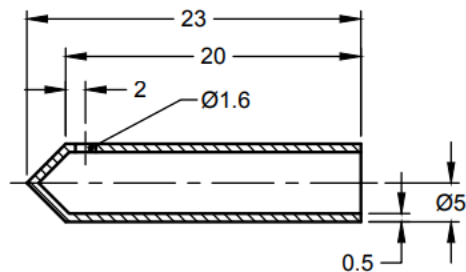

PEN

All dimensions are in millimeters.

FIG. 8B ASSEMBLY AND DETAILS OF PEN

**6.3.8** The recording pen shall not have any lateral play and shall trace the same vertical line on the chart, while going up or coming down, with the drum not rotating.

**6.3.9** Recording raingauges shall have a clockwork mechanism conforming to IS 5924 and capable of running for eight days on one winding. The clockwork shall have a drum shell mounted over it, which shall be friction tight. The drum shell shall be capable of being adjusted for height within a range of 10 mm with respect to the clockwork mechanism. It shall have a flange and a chart clip. Each clockwork shall be provided with an interchangeable winding key.

**6.3.10** The drum diameter and drum height shall conform to the dimensions given in Table 1.

**6.3.11** The recording pen shall traverse on the clock drum, a distance of 276 mm + 1 mm at 27 °C corresponding to 24 h on the chart when the regulator is in the central neutral position. With the regulator at either extreme positions of fast or slow, the distance covered shall be capable of variation by at least one millimeter corresponding to about 5 minutes on the chart.

**6.3.12** The clockwork mechanism shall be so compensated for temperature that the distance traversed by the recording pen in 24 h with regulator at the central neutral position lies between 270 mm and 279 mm for all temperatures between 0°C and 40°C.

**6.3.13** The charts used with recording raingauges shall conform to IS 5947.

## **7 WORKMANSHIP AND FINISH**

**7.1** All parts shall be leak-proof and when assembled the level of the rim of the collector shall be truly horizontal.

**7.2** The external surfaces of the raingauge shall have a smooth and permanent finish.

**7.3** The raingauges shall be of any light colour but a light shade of grass green or cream is preferred [see IS 2932 (Part 1)].

**7.4** All metal parts shall be suitably treated to protect them from rusting or other deterioration.

## **8 DESIGNATION**

For the purposes of inquiry or order, recording raingauges shall be designated by the maximum of the range of rainfall per siphoning as shown in **3** and IS number.

*Example:*

A complete recording raingauge with a range of 0 to 10 mm rainfall per siphoning, conforming to this standard shall be designated as:

Raingauge, Recording 10 mm Rainfall IS 5235

## **9 MARKING**

**9.1** Each raingauge shall bear the following inscription engraved legibly and indelibly on a name plate which shall be cemented firmly on the lid of the float chamber:

- a) Nominal size as fixed in **3**;
- b) Manufacturer's name or recognized trademark; and
- c) Serial number and year of manufacture, for example, No. 123/24.

## **9.2 BIS Certification Marking**

The product(s) conforming to the requirements of this standard may be certified as per the conformity assessment schemes under the provisions of the *Bureau of Indian Standards Act, 2016* and the Rules and Regulations framed thereunder, and the products may be marked with the standard mark.

## **10 PACKING**

Each raingauge without the recording mechanism and clock drum shall be placed in a corrugated cardboard carton with suitable cushioning. The edge of the gun metal rim shall be adequately protected from damage. The recording mechanism and clockwork with drum shell shall be securely packed separately in another corrugated cardboard carton. The two cartons shall be packed in a strong wooden box using suitable packing material. Alternatively, the raingauge shall be packed as agreed to between the supplier and the purchaser.

## **11 TESTING AND INSPECTION**

All raingauges shall be tested individually for conformity to all the requirements of this standard.